



**Crystal Chem**

# **Mouse Total Bile Acids Kit Instructions**

For the quantitative determination of total bile acids  
in mouse serum and plasma

**Catalog #80470  
96 Assays**

**For research use only. Not for use in diagnostic procedures.**

Crystal Chem, Inc.  
1536 Brook Drive, Suite A  
Downers Grove, IL 60515, USA  
Tel: (630) 889-9003 Fax: (630) 889-9021  
E-mail: [sales@crystalchem.com](mailto:sales@crystalchem.com)  
URL: <http://www.crystalchem.com>

# Catalog #80470

## TABLE OF CONTENTS

A. <i>Intended Use</i> .....	1
B. <i>Introduction</i> .....	1
C. <i>Principles of the Assay</i> .....	1
D. <i>Kit Storage</i> .....	1
E. <i>Assay Materials</i>	
E.1. Materials provided.....	1
E.2. Materials to be supplied by user.....	1
F. <i>Assay Precautions</i> .....	2
G. <i>Maximizing Kit Performance</i> .....	2
H. <i>Sample Collection</i> .....	2
I. <i>Assay Procedure</i>	
I.1. Preparation of reagents .....	2
I.2. Preparation of samples, calibrators, and controls .....	2
I.3. Assay procedure .....	3
I.4. Determining the Total Bile Acids concentration .....	3
J. <i>Performance characteristics</i>	
J.1. Assay range .....	4
J.2. Precision .....	4
Warranty.....	4

## Catalog #80470

### **A. Intended Use**

The Mouse Total Bile Acids kit is for the quantitative determination of total bile acids in mouse serum and plasma. The total bile acids concentration is expressed as  $\mu\text{mol/L}$ . Please read the complete kit insert before performing this assay. The kit is for RESEARCH USE ONLY. It is not intended for use in diagnostic procedures.

### **B. Introduction**

Total bile acids is an important test for monitoring normal liver function. Total bile acids are metabolized in the liver and are present in increased concentrations with abnormal liver function.

### **C. Principle of the Assay**

The Mouse Total Bile Acids kit is based on enzymatic technology that utilizes the unique enzymatic property of 3- $\alpha$  hydroxy-steroid dehydrogenase. In the presence of NAD, the bile acids are converted into 3-keto steroids and NADH. The NADH formed reacts with nitrotriazolium blue (NBT) to form a dye. The dye formation is monitored by measuring absorbance at 540nm and is directly proportional to the bile acids concentration in the mouse sample.

### **D. Kit Storage**

1. Upon receipt of the Mouse Total Bile Acids kit, store it at 2-8°C and avoid light exposure (do not freeze the kit or hold it at temperatures above 25°C).
2. The kit should not be used after the expiration date.

### **E. Assay Materials**

#### **E.1. Materials provided**

**TABLE 1 Contents of the kit**

<b>Mark</b>	<b>Description</b>	<b>Amount</b>
CC1	Reagent CC1 (Liquid)	1 X 20 mL
CC2	Reagent CC2 (Liquid)	1 X 4 mL
CC3	Reagent CC3 (Powder)	2 X 10 mL
CAL1	Calibrator 1 (Liquid)	1 X 2 mL

#### **E.2. Materials required but not provided**

Microplates  
Micropipettes and disposable tips  
Clean glass tubes and test tube racks  
Volumetric flasks  
Incubator (37°C)  
Distilled water  
Microplate reader or spectrophotometer or analyzer (should read  $A_{540}$  values)  
0.9% saline

### **F. Assay Precautions**

1. Only appropriately-trained personnel should use the kit. Laboratory personnel should wear suitable protective clothing. All chemicals and reagents should be considered potentially hazardous. Avoid ingestion and contact with skin and eyes.
2. Some assay components contain human & bovine sourced materials. Accordingly, all assay components should be handled as if potentially infectious using safe laboratory procedures.
3. Reagents CC1 and CC2 contain sodium azide, which may react with lead and copper plumbing to form highly explosive metal azide. On disposal, flush with a large volume of water to prevent azide buildup.
4. Do not use the reagents after the expiration date.

### **G. Maximizing Kit Performance**

1. Given the small sample volumes required (20  $\mu$ L), pipetting should be done as carefully as possible. A high quality 50  $\mu$ L or better precision pipette should be used for such volumes. Drops of liquid adhering to the outside of the pipette tips should be removed by wiping to ensure the highest degree of accuracy.
2. In order to prevent the microplate wells from drying out and to get the best results, samples and reagents should be dispensed quickly into the wells.
3. Each calibrator and sample should be assayed in duplicate.
4. The same sequence of pipetting and other operations should be maintained in all procedures.
5. Do not mix reagents that have different lot numbers.

### **H. Sample Collection**

Fresh serum or EDTA treated plasma samples should be used. Hemolysed or heparinized samples should not be used.

***Note:** Samples should be collected under fasting conditions as total bile acid concentrations increase after meals. It is recommended that samples be used within 1 week of collection when stored refrigerated. If assay is to be performed more than 1 week after collection, samples should be frozen.*

### **I. Assay Procedure**

#### **I.1. Preparation of reagents**

Prior to running the assay, Reagent CC3 must be reconstituted using Reagent CC1. Add 10 mL of Reagent CC1 to one bottle of Reagent CC3 and dissolve by swirling gently. Reconstituted Reagent CC3 is stable for 1 week at 2-8°C.

All reagents should be stored at 2-8°C immediately after use. Do not freeze reagents, calibrators, or controls. Before use, bring all reagents to room temperature and mix the reagents thoroughly by gentle agitation or swirling.

#### **I.2. Preparation of samples, calibrators, and controls**

1. Bring all samples, calibrators, and controls to room temperature. Frozen samples should be allowed to fully thaw before proceeding.


***Note:** In addition to running the calibrator provided, the assay requires running a blank calibrator. Distilled water should be used for running the blank calibrator. Optional controls are sold separately (Cat# 80473). Controls should be reconstituted with 1 mL of H<sub>2</sub>O.*

### I.3. Assay procedure

The procedure below reflects a manual procedure performed using a microplate and a microplate reader (ideal when running multiple samples manually). The procedure can be easily adopted as needed to be run in a glass tube with a spectrophotometer. The assay can also be adopted to work on various automated analyzers using the schema presented in Figure 1. Please contact Crystal Chem for instrument-specific information.

1. Add 150  $\mu\text{L}$  of reconstituted Reagent CC3 and 20  $\mu\text{L}$  of sample, calibrator, or control into each well (as needed) of a microplate and mix well by repeated pipetting.
2. Place microplate in incubator ( $37^{\circ}\text{C}$ ) and allow microplate to equilibrate to  $37^{\circ}\text{C}$  over 5 minutes.
3. Zero the absorbance of plate reader at 540nm.
4. Measure absorbance using a plate reader (measure  $A_{540}$  values).  
*Note: The Mouse Total Bile Acids assay is an end-point assay and the first reading point A1 is right before the addition of reagent CC2.*
5. Add 30  $\mu\text{L}$  of Reagent CC2 and mix well by repeated pipetting.
6. Measure the increase in absorbance after 5 minutes at  $37^{\circ}\text{C}$  using a plate reader (measure  $A_{540}$  values).

**Figure 1. Summary of assay procedure**

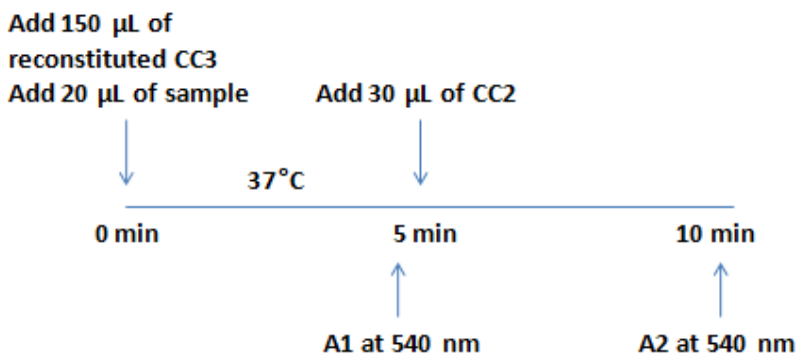

### I.4. Determining the mouse total bile acids concentration

1. Calculate the change in absorbance  $\Delta A$  (0sec ~ 300sec) for each well.

$$\Delta A = (OD_{540\text{nm}, 300\text{sec}}) - (OD_{540\text{nm}, 0\text{sec}})$$

2. Using linear graph paper, construct the total bile acids calibration curve by plotting the mean change in absorbance value for the calibrator (incl. blank) on the Y axis versus the corresponding total bile acids concentration on the X axis.  
**Note:** Calibrator value varies per lot and should be obtained from the calibrator label. The calibrator and blank should be run every time the assay is performed.

## Catalog #80470

3. Mouse total bile acid concentrations in the samples are interpolated using the calibration curve and mean change in absorbance values for each sample. The total bile acids concentration is expressed as  $\mu\text{mol/L}$ . This interpolation can be simplified using Equation 1 below.

**Note:** *Samples with a high total bile acids concentration (180  $\mu\text{mol/L}$  or higher) should be diluted with the 0.9% saline and rerun.*

### **Equation 1. Calculation of mouse total bile acids concentration**

*Mouse BA concentration =*

$$[(\text{sample } A_{540} - \text{blank } A_{540}) / (\text{calibrator } A_{540} - \text{blank } A_{540})] \times \text{calibrator conc.}$$

### **J. Performance characteristics**

#### **J.1. Assay range**

The Mouse Total Bile Acids assay has a linear range from 0-180  $\mu\text{mol/L}$ .

#### **J.2. Precision**

The assay has a within-run and total precision of CV < 10%.

### **Warranty**

Crystal Chem Inc. makes no warranty of any kind, either expressed or implied, except that the materials from which its products are made are of standard quality. Buyer assumes all risk and liability resulting from the use of this product.

**THERE IS NO WARRANTY OF MERCHANTABILITY OF THE PRODUCTS, OR THAT SUCH PRODUCTS ARE FIT FOR ANY PARTICULAR PURPOSE. CRYSTAL CHEM INC'S LIABILITY SHALL NOT EXCEED THE RETURN OF THE PURCHASE PRICE, AND UNDER NO CIRCUMSTANCES SHALL CRYSTAL CHEM INC. BE LIABLE FOR SPECIAL OR CONSEQUENTIAL DAMAGES, OR EXPENSES ARISING DIRECTLY OR INDIRECTLY FROM THE USE OF THIS PRODUCT.**