



Aviva Systems Biology Corporation
7700 Ronson Rd, Suite 100
San Diego, CA 92111
Tel: 858-552-6979 Fax: 858 -552-6975
Email: info@avivasysbio.com
Web: www.avivasysbio.com

CERTIFICATE OF ANALYSIS

Product: Human ACHE ELISA Kit

Catalog No: OKEH00857

Lot No: KE0593

Expiration Date: 2020.11

Performance Characteristics:

Intra-Assay CV	< 6.3%	Passed
Inter-Assay CV	< 10.4%	Passed
Limit of Detection (LOD)		< 0.1 ng/mL
Assay Range		0.312 – 20 ng/mL

Standard Dilution:


Prepare the standards immediately before use. For each experiment, add 2 mL of Sample Diluent to the 80 ng Lyophilized ACHE Standard. Mix gently until dissolved. Leave the vial at ambient temperature for 15 minutes.

Prepare a 20 ng/mL Standard by adding 500 µL of 40 ng/mL Standard to 500 µL of Sample Diluent in Tube #1. Mix gently and thoroughly.

Standard Number (Tube)	Standard to Dilute	Volume Standard to Dilute (µL)	Volume Sample Diluent (µL)	Total Volume (µL)	Final Concentration (ng/mL)
Standard	80 ng/mL ACHE Standard	NA	2,000	2,000	40 ng/mL
1	40 ng/mL	500	500	1,000	20 ng/mL
2	20 ng/mL	300	300	600	10 ng/mL
3	10 ng/mL	300	300	600	5.0 ng/mL
4	5.0 ng/mL	300	300	600	2.5 ng/mL
5	2.5 ng/mL	300	300	600	1.25 ng/mL
6	1.25 ng/mL	300	300	600	0.625 ng/mL
7	0.625 ng/mL	300	300	600	0.312 ng/mL
8	N/A	0	300	300	0.0 (Blank)

Sample Standard Curve and Calculations ONLY. Do not use below report for result calculations. A standard curve should be generated each time the test is performed

Standard Curve Graph

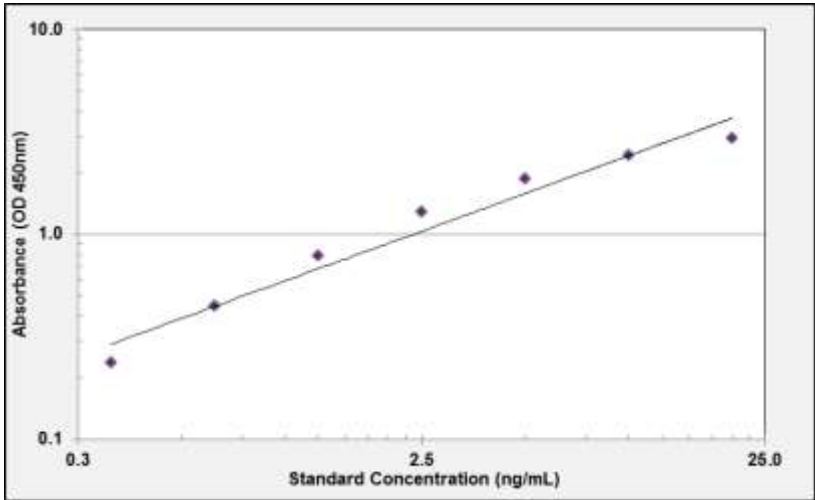

Standard ng/mL	Absorbance (OD 450nm)
20	2.919
10	2.399
5.0	1.840
2.5	1.276
1.25	0.773
0.625	0.440
0.312	0.233