

Anti-PIAS1+PIAS2+PIAS3 Rabbit Monoclonal Antibody

Catalog Number: M01707

About PIAS1

Furin is likely to represent the ubiquitous endoprotease activity within constitutive secretory pathways and capable of cleavage at the RX (K/R) R consensus motif.

Overview

Product Name	Anti-PIAS1+PIAS2+PIAS3 Rabbit Monoclonal Antibody
Reactive Species	Human, Mouse, Rat
Description	Boster Bio Anti-PIAS1+PIAS2+PIAS3 Rabbit Monoclonal Antibody catalog # M01707. Tested in WB, IHC, ICC/IF, IP, Flow Cytometry applications. This antibody reacts with Human, Mouse, Rat.
Application	Flow Cytometry, IP, IF, IHC, ICC, WB
Clonality	Monoclonal ABFA-16
Formulation	Rabbit IgG in phosphate buffered saline, pH 7.4, 150mM NaCl, 0.02% sodium azide and 50% glycerol, 0.4-0.5mg/ml BSA.
Storage Instructions	Store at -20°C for one year. For short term storage and frequent use, store at 4°C for up to one month. Avoid repeated freeze-thaw cycles.
Host	Rabbit
Uniprot ID	O75925/O75928

Technical Details

Immunogen	A synthesized peptide derived from human PIAS1+PIAS2+PIAS3
Isotype	Rabbit IgG
Form	Liquid
Concentration	Actual concentration vary by lot. Use suggested dilution ratio to decide dilution procedure.
Purification	Affinity-chromatography
Suggested Dilutions	Dilute the sample so that the expected range of concentrations fall within the detection range of this kit. If the expected range of concentration is unknown, a pilot test should be conducted to decide the optimal dilution ratio for your samples. Some PubMed article(s) citing the expression level of this target are as follows: Boster Bio's internal QC testing used: WB 1:500-1:2000

	IHC 1:50-1:200 ICC/IF 1:50-1:200 IP 1:50 FC 1:50
--	---

Anti-PIAS1+PIAS2+PIAS3 Rabbit Monoclonal Antibody (M01707) Images

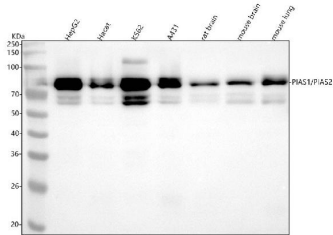


Figure 1. Western blot analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707).

Electrophoresis was performed on a 5-20% SDS-PAGE gel at 70V (Stacking gel) / 90V (Resolving gel) for 2-3 hours. The sample well of each lane was loaded with 30 ug of sample under reducing conditions.

Lane 1: human HepG2 whole cell lysates,

Lane 2: human Haca whole cell lysates,

Lane 3: human K562 whole cell lysates,

Lane 4: human A431 whole cell lysates,

Lane 5: rat brain tissue lysates,

Lane 6: mouse brain tissue lysates,

Lane 8: mouse lung tissue lysates.

After electrophoresis, proteins were transferred to a nitrocellulose membrane at 150 mA for 50-90 minutes. Blocked the membrane with 5% non-fat milk/TBS for 1.5 hour at RT. The membrane was incubated with rabbit anti-PIAS1+PIAS2+PIAS3 antigen affinity purified monoclonal antibody (Catalog # M01707) at 1:500 overnight at 4°C,

then washed with TBS-0.1%Tween 3 times with 5 minutes each and probed with a goat anti-rabbit IgG-HRP secondary antibody at a dilution of 1:5000 for 1.5 hour at RT. The signal is developed using an Enhanced Chemiluminescent detection (ECL) kit (Catalog # EK1002) with Tanon 5200 system. A specific band was detected for PIAS1+PIAS2+PIAS3 at approximately 76 kDa. The expected band size for PIAS1+PIAS2+PIAS3 is at 76 kDa.

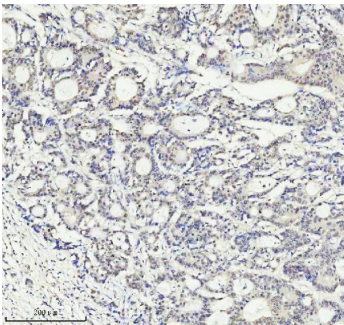


Figure 2. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707).

PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of human colon adenocarcinoma tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

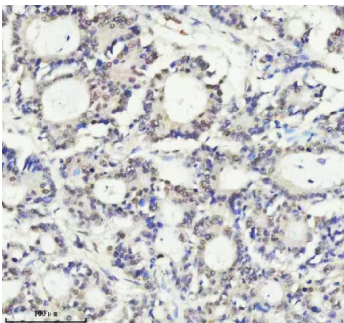


Figure 3. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707).

PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of human colon adenocarcinoma tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was

developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

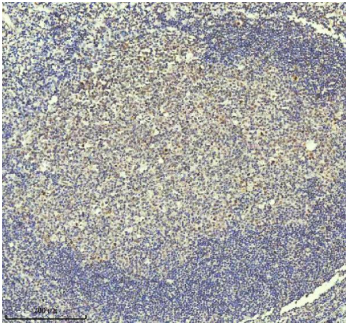


Figure 4. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707). PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of human spleen tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

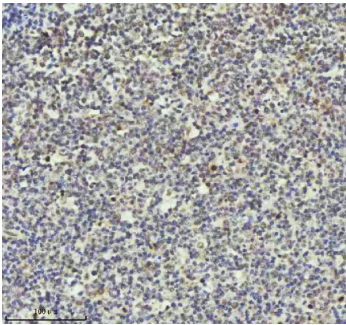


Figure 5. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707). PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of human spleen tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

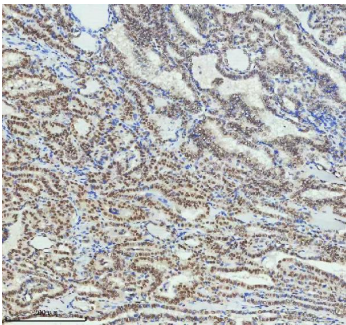


Figure 6. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707). PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of human thyroid papillary carcinoma tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

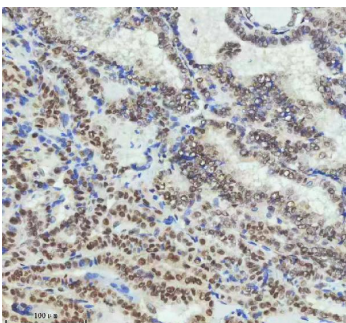


Figure 7. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707). PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of human thyroid papillary carcinoma tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was

developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

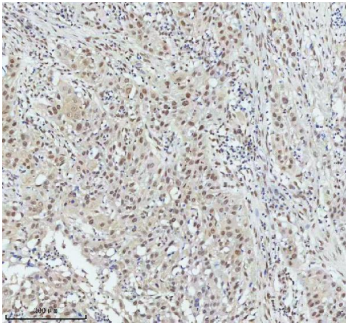


Figure 8. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707). PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of human urothelial carcinoma tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

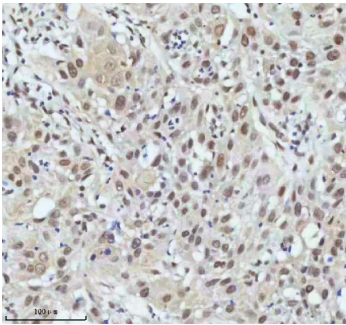


Figure 9. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707). PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of human urothelial carcinoma tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

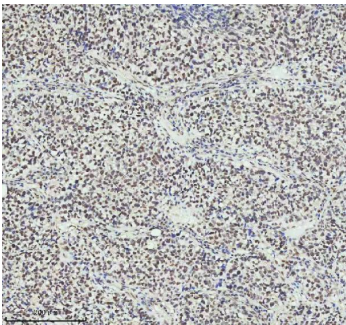


Figure 10. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707). PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of non-small cell lung cancer tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

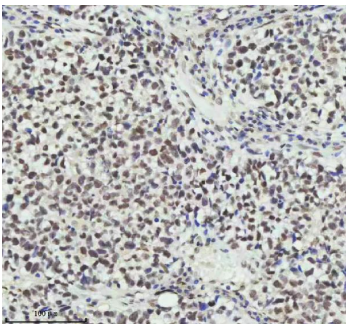


Figure 11. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707). PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of non-small cell lung cancer tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was developed using

HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

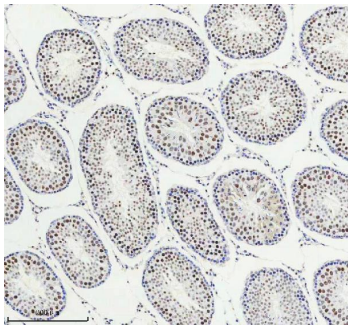


Figure 12. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707). PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of rat testis tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

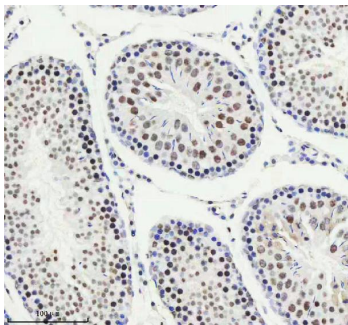


Figure 13. IHC analysis of PIAS1+PIAS2+PIAS3 using anti-PIAS1+PIAS2+PIAS3 antibody (M01707). PIAS1+PIAS2+PIAS3 was detected in a paraffin-embedded section of rat testis tissue. Heat mediated antigen retrieval was performed in EDTA buffer (pH 8.0, epitope retrieval solution). The tissue section was blocked with 10% goat serum. The tissue section was then incubated with 1:50 rabbit anti-PIAS1+PIAS2+PIAS3 Antibody (M01707) overnight at 4°C. Peroxidase Conjugated Goat Anti-rabbit IgG was used as secondary antibody and incubated for 30 minutes at 37°C. The tissue section was developed using HRP Conjugated Rabbit IgG Super Vision Assay Kit (Catalog # SV0002) with DAB as the chromogen.

Submit a product review to Biocompare.com

Submit a review of this product to Biocompare.com to receive a \$20 Amazon.com giftcard! Your reviews help your fellow scientists make the right decisions. Thank you for your contribution.



Anti-PIAS1+PIAS2+PIAS3 Rabbit Monoclonal Antibody