





Human Fibrinogen(FB) ELISA Kit

| Product Code | CSB-E13656h | | | | |
|---------------------------------------|---|---|---|--|--|
| Abbreviation | Fb | | | | |
| Target Name | Fibrinogen(FB) | | | | |
| Alias | N/A | | | | |
| Product Type | ELISA Kit | | | | |
| Immunogen Species | Homo sapiens (Human) | | | | |
| Sample Types | serum, plasma, tissue homogenates | | | | |
| Detection Range | 0.312 μg/mL-20 μg/mL | | | | |
| Sensitivity | 0.078 μg/mL | | | | |
| Assay Time | 1-5h | | | | |
| Sample Volume | 50-100ul | | | | |
| Detection Wavelength | 450 nm | | | | |
| Lead Time | 3-5 working days after you place the order, and it takes another 3-5 days for delivery via DHL or FedEx. | | | | |
| Research Area | Cardiovascular | | | | |
| Tag Info | quantitative | | | | |
| | Sandwich | | | | |
| Protein Description | Sandwich | | | | |
| Protein Description Description | This Human F measurement homogenates. | of Human Fibrinogen (| Kit was designed for the quantitative FB) protein in serum, plasma, tissue A kit, its detection range is 0.312 μg/mL-20 mL. | | |
| · · · · · · · · · · · · · · · · · · · | This Human F measurement homogenates. µg/mL and the Intra-assay Pr Three sample to assess. Inter-assay Pr | of Human Fibrinogen (I It is a Sandwich ELISA e sensitivity is 0.078 μg/ recision (Precision withing s of known concentration | FB) protein in serum, plasma, tissue A kit, its detection range is 0.312 μg/mL-20 mL. | | |







| 1:400 | Average % | 97 |
|-------|-----------|--------|
| 1.400 | Range % | 90-105 |
| 1:800 | Average % | 93 |
| 1.000 | Range % | 86-98 |


Recovery

The recovery of human FB spiked to levels throughout the range of the assay in various matrices was evaluated. Samples were diluted prior to assay as directed in the Sample Preparation section.

| Sample Type | Average % Recovery | Range |
|-------------------|--------------------|--------|
| Serum (n=5) | 92 | 87-98 |
| EDTA plasma (n=4) | 98 | 90-106 |

Typical

These standard curves are provided for demonstration only. A standard curve should be generated for each set of samples assayed.

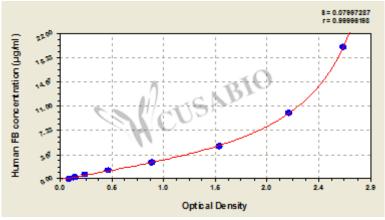

μg/ml OD1 OD2 Average Corrected

| . • | | • | |
|-------|-------------|-------|-------|
| 20 | 2.648 2.701 | 2.675 | 2.583 |
| 10 | 2.159 2.169 | 2.164 | 2.072 |
| 5 | 1.476 1.536 | 1.506 | 1.414 |
| 2.5 | 0.864 0.876 | 0.870 | 0.778 |
| 1.25 | 0.443 0.475 | 0.459 | 0.367 |
| 0.625 | 0.234 0.253 | 0.244 | 0.152 |
| 0.312 | 0.146 0.154 | 0.150 | 0.058 |
| 0 | 0.095 0.089 | 0.092 | ? |
| | | | |

Msds

{"0":{"fileurl":"https://www.cusabio.com/uploadfile/msds/MSDS CSB-E13656h.pdf","filename":"MSDS"}}