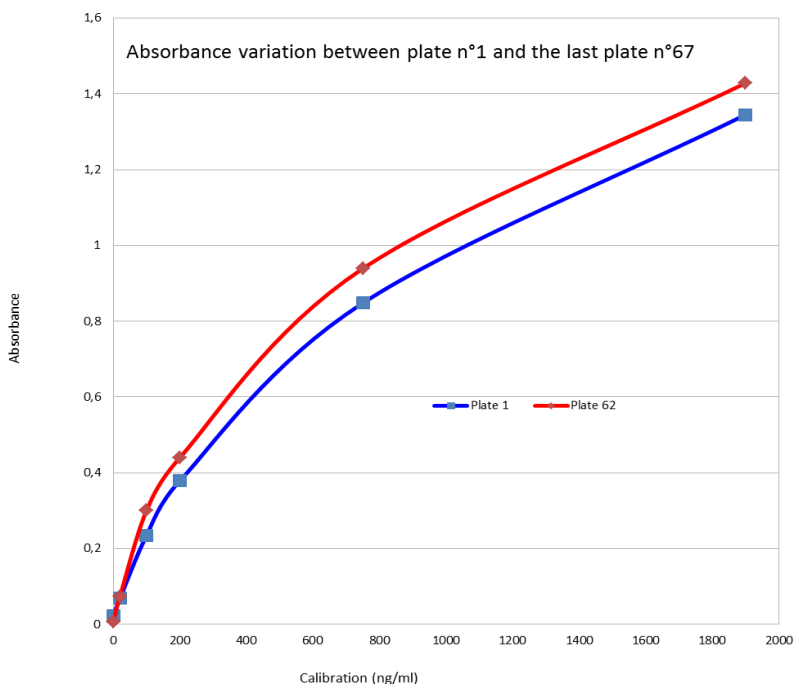


Certificate of Analysis

Kit	IgG Mouse ELISA Quantification Kit
Code	RDB-3256-10
Batch	1904A
Expiry date	01/2020

Shelfe life: Calibration range: Detection limit: Hook effect:	<p>One year at +4°C, two months after opening</p> <p>From 20 ng/ml up to 1900 ng/ml</p> <p>6 ng/ml</p> <p>A hook effect is generally observed at IgG concentration above 3000 ng/ml. Dilution of sample is then recommended.</p>
Quality control: <p>Absorbance variation between plate n°1 and the last plate n°62 should be below 10% → Passes Test</p>	 <p>Absorbance variation between plate n°1 and the last plate n°62</p>
Batch release:	<p>This product has been fully tested and is deemed functional by Quality Control.</p> <p>Date: 12/04/2019, Thomas Taillard</p> 