

# Human Lipocalin-2/LCN2 ELISA Pair Set

Catalog Number: SEK10222

To achieve the best assay results, this manual must be read carefully before using this product and the assay is run as summarized in the General ELISA protocol.

#### BACKGROUND

Lipocalin-2 (LCN2), also known as neutrophil gelatinase-associated lipocalin (NGAL), is a 25 kDa protein belonging to the lipocalin superfamily. It was initially found in activated neutrophils, however, many other cells, like kidney tubular cells, may produce NGAL in response to various insults. This protein is released from injured tubular cells after various damaging stimuli, is already known by nephrologists as one of the most promising biomarkers of incoming Acute Kidney Injury (AKI). Recent evidence also suggests its role as a biomarker in a variety of other renal and non-renal conditions. Moreover, recent studies seem to suggest a potential involvement of this factor also in the genesis and progression of chronic kidney diseases. NGAL is the first known mammalian protein which specifically binds organic molecules called siderophores, which are high-affinity iron chelators. NGAL, first known as an antibacterial factor of natural immunity, and an acute phase protein, is currently one of the most interesting and enigmatic proteins involved in the process of tumor development, acting as an intracellular iron carrier and protecting MMP9 from proteolytic degradation, NGAL has a clear pro-tumoral effect, as has already been observed in different tumors (e.g. breast, stomach, oesophagus, brain) in humans. In thyroid carcinomas, NGAL is strongly induced by NF-kB, an important factor involved both in tumor growth and in the link between chronic inflammation and neoplastic development. Thus, Lipocalin-2 (LCN2/NGAL) has been implicated in a variety of processes including cell differentiation, proliferation, survival and morphogenesis.


#### PRINCIPLE OF THE TEST

The Sino Biological ELISA Pair Set is a solid phase sandwich ELISA (Enzyme-Linked Immunosorbent Assay). It utilizes a monoclonal antibody specific for Human Lipocalin-2/LCN2 coated on a 96-well plate. Standards and samples are added to the wells, and any Human Lipocalin-2/LCN2 present binds to the immobilized antibody. The wells are washed and a horseradish peroxidase conjugated mouse anti-Human Lipocalin-2/LCN2 monoclonal antibody is then added, producing an antibody-antigen-antibody "sandwich". The wells are again washed and TMB substrate solution is loaded, which produces color in proportion to the amount of Human Lipocalin-2/LCN2 present in the sample. To end the enzyme reaction, the stop solution is added and absorbances of the microwell are read at 450 nm.

#### **INTENDED USE**

- ◆The Human Lipocalin-2/LCN2 ELISA Pair Set is for the quantitative determination of Human Lipocalin-2/LCN2.
- ◆This ELISA Pair Set contains the basic components required for the development of sandwich ELISAs.

# **ASSAY PROCEDURE SUMMARY**

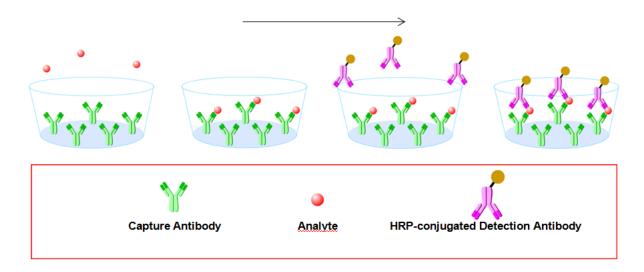

This Pair Set has been configured for research use only and is not to be used in diagnostic procedures.

# MATERIALS PROVIDED

Bring all reagents to room temperature before use.

**Capture Antibody** – 1 mg/mL of mouse anti-Human Lipocalin-2/LCN2 monoclonal antibody (in PBS, pH 7.4). Dilute to a working concentration of 0.5  $\mu$ g/mL in PBS before coating. (Catalog: # 10222-MM03)

**Detection Antibody** - 0.2 mg/mL of mouse anti-Human Lipocalin-2/LCN2 monoclonal antibody conjugated to horseradish-peroxidase (HRP) (in PBS, 50 % HRP-Protector, pH 7.4, store at  $4^{\circ}$ C). Dilute to working concentration of 0.05 µg/mL in detection antibody dilution buffer before use. (Catalog: # 10222-MM18)

**Standard** – Each vial contains 300 ng of recombinant Human Lipocalin-2/LCN2. Reconstitute with 1 mL detection antibody dilution buffer. After reconstitution, store at -20°C to -80°C in a manual defrost freezer. A seven-point standard curve using 2-fold serial dilutions in sample dilution buffer, and a high standard of 10000 pg/mL is recommended.

## SOLUTIONS REQUIRED

**PBS** - 136.9 mM NaCl, 10.1 mM Na $_2$ HPO $_4$ , 2.7 mM KCl, 1.8 mM KH $_2$ PO $_4$ , pH 7.4, 0.2  $\mu$ m filtered

Wash Buffer - 0.05% Tween20 in PBS, pH 7.2 - 7.4

**Blocking Buffer** - 2% BSA in Wash Buffer

Sample dilution buffer - 0.1% BSA in wash buffer, pH 7.2 - 7.4, 0.2 µm filtered

Detection antibody dilution buffer - 0.5% BSA in wash buffer, pH 7.2 - 7.4, 0.2 µm filtered

Substrate Solution: To achieve best assay results, fresh substrate solution is recommended

Substrate stock solution - 10mg / ml TMB ( Tetramethylbenzidine ) in DMSO

Substrate dilution buffer - 0.05M Na<sub>2</sub>HPO<sub>4</sub> and 0.025M citric acid; adjust pH to 5.5

Substrate working solution - For each plate dilute 250  $\mu$ l substrate stock solution in 25ml substrate dilution buffer and then add 80  $\mu$ l 0.75%  $H_2O_2$ , mix it well

Stop Solution - 2 N H<sub>2</sub>SO<sub>4</sub>

# **PRECAUTION**

The Stop Solution suggested for use with this Pair Set is an acid solution. Wear eye, hand, face, and clothing protection when using this material.

# STORAGE

**Capture Antibody**: Aliquot and store at  $-20^{\circ}$ C to  $-80^{\circ}$ C for up to 6 months from date of receipt. Avoid repeated freeze-thaw cycles.

**Detection Antibody**: Store at  $4^{\circ}$ C and protect it from prolonged exposure to light for up to 6 months from date of receipt. **DO NOT FREEZE!** 

**Standard**: Store lyophilized standard at  $-20^{\circ}$ C to  $-80^{\circ}$ C for up to 6 months from date of receipt. Aliquot and store the reconstituted standard at  $-80^{\circ}$ C for up to 1 month. Avoid repeated freeze-thaw cycles.

#### GENERAL ELISA PROTOCOL

#### **Plate Preparation**

- 1.Dilute the capture antibody to the working concentration in PBS. Immediately coat a 96-well microplate with 100 $\mu$ L per well of the diluted capture antibody. Seal the plate and incubate overnight at 4°C.
- 2.Aspirate each well and wash with at least 300µl wash buffer, repeating the process two times for a total of three washes. Complete removal of liquid at each step is essential for good performance. After the last wash, remove any remaining wash buffer by inverting the plate and blotting it against clean paper towels.
- 3.Block plates by adding 300  $\mu$ L of blocking buffer to each well. Incubate at room temperature for a minimum of 1 hour.
- 4.Repeat the aspiration/wash as in step 2. The plates are now ready for sample addition.

# **Assay Procedure**


- 1.Add 100  $\mu$ L of sample or standards in sample dilution buffer per well. Seal the plate and incubate 2 hours at room temperature.
- 2. Repeat the aspiration/wash as in step 2 of plate preparation.
- 3.Add 100  $\mu$ L of the detection antibody, diluted in antibody dilution buffer, to each well. Seal the plate and incubate 1 hour at room temperature.
- 4. Repeat the aspiration/wash as in step 2 of plate preparation.
- $5.Add\ 200\ \mu L$  of substrate solution to each well. Incubate for 20 minutes at room temperature ( if substrate solution is not as requested, the incubation time should be optimized ). Avoid placing the plate in direct light.
- 6.Add 50 µL of stop solution to each well. Gently tap the plate to ensure thorough mixing.
- 7. Determine the optical density of each well immediately, using a microplate reader set to 450 nm.

#### CALCULATION OF RESULTS

- •Calculate the mean absorbance for each set of duplicate standards, controls and samples. Subtract the mean zero standard absorbance from each.
- •Construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph.
- •To determine the concentration of the unknowns, find the unknowns' mean absorbance value on the y-axis and draw a horizontal line to the standard curve. At the point of intersection, draw a vertical line to the x-axis and read the concentration. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.
- •Alternatively, computer-based curve-fitting statistical software may also be employed to calculate the concentration of the sample.

#### **TYPICAL DATA**

This standard curve is only for demonstration purposes. A standard curve should be generated for each assay.

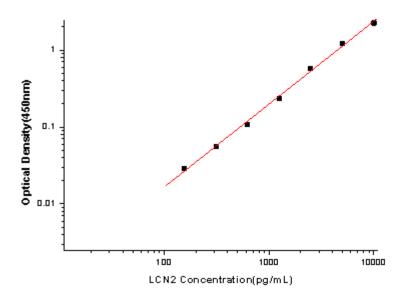

Concentration ( pg/mL)	Zero standard subtracted OD			
0	0			
156.25	0.029			
312.50	0.056			
625	0.108			
1250	0.236			
2500	0.577			
5000	1.226			
10000	2.244			

#### PERFORMANCE CHARACTERISTIC

## SENSITIVITY

The minimum detectable dose of Human Lipocalin-2/LCN2 was determined to be approximately **156.25 pg/ml**. This is defined as at least three times standard deviations above the mean optical density of 10 replicates of the zero standard.

# TROUBLE SHOOTING

Problems	Possible Sources	Solutions			
	Incorrect or no Detection Antibody was added	Add appropriate Detection Antibody and continue			
No signal	Substrate solution was not added	Add substrate solution and continue			
	Incorrect storage condition	Check if the kit is stored at recommended condition and used before expiration date			
Poor Standard Curve	Standard was incompletely reconstituted or was inappropriately stored	Aliquot reconstituted standard and store at -80 $^{\circ}\mathrm{C}$			
	Imprecise / inaccurate pipetting	Check / calibrate pipettes			
	Incubations done at inappropriate temperature, timing or agitation	Follow the general ELISA protocol			
	Background wells were contaminated	Avoid cross contamination by using the sealer appropriately			
	The concentration of antigen in samples was too low	Enriching samples to increase the concentration of antigen			
Poor detection value	Samples were ineffective	Check if the samples are stored at cold environment. Detect samples in timely manner			
	Insufficient washes	Use multichannel pipettes without touching the reagents on the plate			
	insunicient wasnes	Increase cycles of washes and soaking time between washes			
High Background	TMB Substrate Solution was contaminated	TMB Substrate Solution should be clear and colorless prior to addition to wells			
	Materials were contaminated.	Use clean plates, tubes and pipettes tips			
Non-specificity	Samples were contaminated	Avoid cross contamination of samples			
	The concentration of samples was too high	Try higher dilution rate of samples			

	12								
ELISA Plate Template	11								
	10								
	0								
	œ								
	7								
	9								
	Ŋ								
	4								
	m								
	7								
	-								
		4	8	U	۵	ш	<b>L</b>	U	I

# Human Lipocalin-2/LCN2 ELISA Pair Set Notes